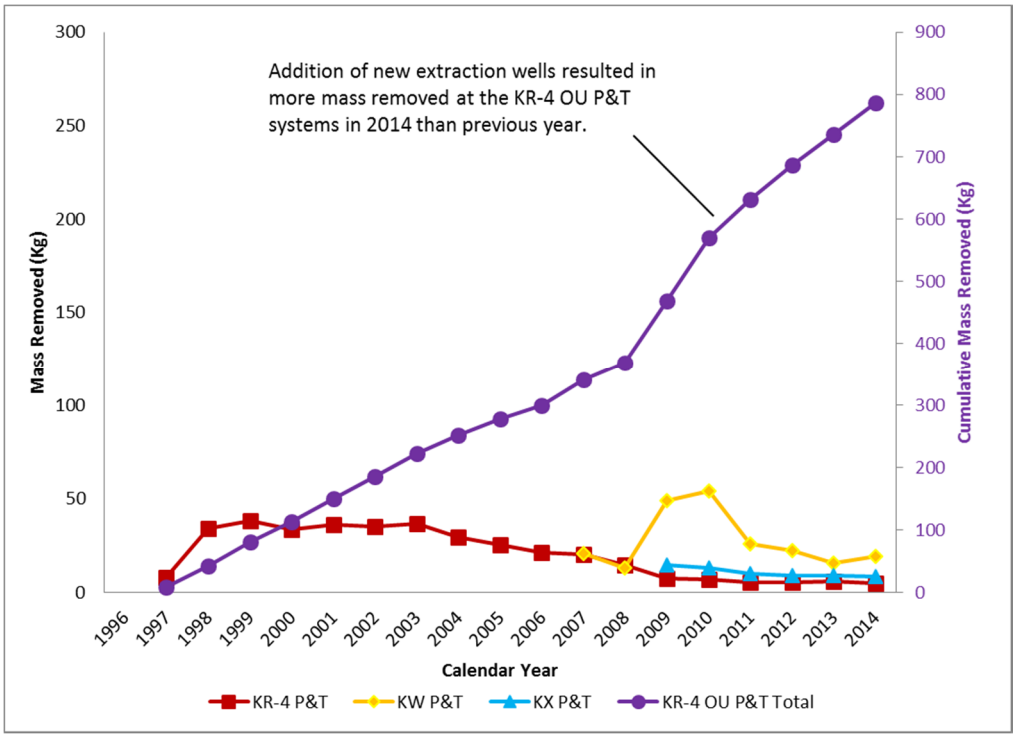

Figure 1-9. Cr(VI) Mass Removed by the 100-KR-4 OU P&T Systems